

9025 Technology Dr. • Fishers, IN 46038-2886
800.387.0672 • 317.570.7020 • Fax 317.570.7034
info@bangslabs.com • www.bangslabs.com

Bangs Laboratories, Inc.

BEADS ABOVE THE REST™

DESCRIPTION

Vivaspin® Concentrators are disposable ultrafiltration devices that may be utilized for the washing and concentration of submicron (20 nm - 0.5 µm) microspheres.

Vivaspin® 2 can effectively be used in either swing bucket or fixed angle rotor centrifuges accepting 15 mL tubes. The patented vertical membrane design and thin channel filtration chamber (US 5,647,990) minimizes membrane fouling and provides high speed concentrations, even with particle laden solutions. The proven high flux polyethersulfone (PES) membrane range is recommended with most solutions (*see Table 2 for chemical compatibility*).

APPLICATIONS

The Vivaspin® 2 is specifically designed with low internal surface and membrane area in order to achieve superior recoveries from very dilute solutions. Another feature of the Vivaspin® 2 is the choice of directly pipetting the concentrate from the dead stop pocket built into the bottom of the concentrator, or alternatively reverse spinning the concentrate into the recovery cap which can then be sealed for storage.

TECHNICAL SPECIFICATIONS

Table 1:

Concentrator capacity	
Swing bucket rotor	3 mL
Fixed angle rotor	2 mL
Dimensions	
Total length	126 mm
Width	17 mm
Active membrane area	1.2 cm ²
Hold-up volume membrane and support	<10 µL
Dead stop volume	8 µL
Materials of construction	
Body	Polycarbonate
Filtrate vessel	Polycarbonate
Concentrator cap	Polycarbonate
Membrane	PES

* Dead stop volume as designed in moulding tool. This volume may vary depending on sample, sample concentration, operation temperature and centrifuge rotor.

EQUIPMENT REQUIRED

1. Centrifuge with swing bucket or fixed angle (minimum 25°) rotor (carrier required: 15 mL/17mmd)
2. Pipettes for sample delivery and removal. For maximum recovery a thin gel loader type is recommended.



PROCEDURE

1. This Vivaspin® 2mL device features a 300,000 MWCO Polyethersulfone (PES) membrane. It is suitable for retaining particles 20nm+.
2. Fill concentrator body with up to maximum volumes in Table 1. (Ensure lid is fully seated). The microsphere sample may be diluted prior to loading.

Notes - Removing the Vivaspin® 2 body from the filtrate tube


- a. The base of the concentrator body (seen from the end) is oval in cross section. The filtrate tube is round in cross section to give a tight fit to the concentrator body. To release the tube from the concentrator body, you must pinch the tube – before removing it with a twisting action.
- b. After each round of centrifugation, the device may be bath sonicated briefly (~30 seconds) to deter sticking of the particles to the membrane.

3. Insert assembled concentrator into centrifuge (when fixed angle rotors are used, angle concentrator so that the printed window faces upwards/outwards).
4. Centrifuge at 3,000 - 4,500 × G for 5-10 minutes (or 4000 × G for swing bucket rotors). The aim is to concentrate the particle - containing fraction, but not form a pellet. For example, one wash might begin with 2 mL suspension, and concentrate to 0.2 mL.
5. Filtrate may be discarded or decanted from the base of the device.
6. Repeat washes by adding more buffer to the concentrator body, and then centrifuging, and decanting filtrate. Typically three wash cycles are conducted. After each separation, the assembled device may be held in a sonicator briefly (30 sec.) Care should be taken to ensure that water from the bath sonicator is not introduced into the device.
7. Pipet concentrate from the dead stop pocket in the bottom of the concentrator. It is also possible to reverse spin the device to maximize recovery (*see reverse spin instructions*).

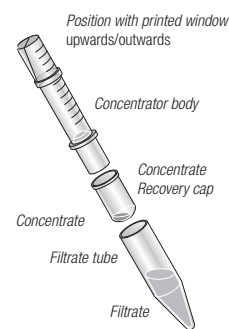

REVERSE SPIN WITH VIVASPIN® 2

Depending on user preference and need for sample storage, the concentrate can be reverse spun into the concentrate recovery cap (when fixed angle rotors are used, angle concentrator so that the printed window faces upwards/outwards). In this procedure remove filtrate tube, invert the concentrator body, insert concentrate recovery cap into filtrate tube and then spin at up to 3,000 ×G for 2 minutes. The concentrate recovery cap can be sealed for storage.



Usage Tips

- Flow Rate** - Filtration rate is affected by several parameters, including MWCO, porosity, sample concentration, viscosity, centrifugal force and temperature. Expect significantly longer spin times for starting solutions with over 5% solids. When operating at 4°C, flow rates are approximately 1.5 times slower than at 25°C. Viscous solutions such as 50% glycerine will take up to 5 times longer to concentrate than samples in a predominantly buffer solution.
- Pre-rinsing** - Membranes fitted to Vivaspin® concentrators contain trace amounts of Glycerine and Sodium azide. Should these interfere with analysis they can be removed by rinsing fill volume of buffer solution or deionized water through the concentrator. Decant filtrate and concentrate before processing sample solution. If you do not want to use the pre-rinsed device immediately, store it in the refrigerator with buffer or water covering the membrane surface. Do not allow the membrane to dry out.
- Sterilization of Polyethersulfone Membranes** - Vivaspin® devices should not be autoclaved as high temperatures will substantially increase membrane MWCO. To sterilize, use a 70% ethanol solution or sterilizing gas mixture.
- Chemical Compatibility** - Vivaspin® concentrators are designed for use with biological fluids and aqueous solutions. For chemical compatibility details, refer to Table 2.

CHEMICAL COMPATIBILITY (2hr contact time)

Table 2:

Solutions	
Compatible pH range	pH 1–9
Acetic Acid (25.0%)	OK
Acetone (10.0%)	NO
Acetonitrile (10.0%)	NO
Ammonium Hydroxide (5.0%)	?
Ammonium Sulphate (saturated)	OK
Benzene (100%)	NO
n-Butanol (70%)	?
Chloroform (1.0%)	NO
Dimethyl Formamide (10.0%)	?
Dimethyl Sulfoxide (5.0%)	OK
Ethanol (70.0%)	OK
Ethyl Acetate (100%)	NO
Formaldehyde (30%)	OK
Formic Acid (5.0%)	OK

Glycerine (70%)	OK
Guanidine HCl (6 M)	OK
Hydrocarbons, aromatic	NO
Hydrocarbons, chlorinated	NO
Hydrochloric Acid (1 M)	OK
Imidazole (300 mM)	OK
Isopropanol (70%)	OK
Lactic Acid (5.0%)	OK
Mercaptoethanol (1.0 M)	NO
Methanol (60%)	?
Nitric Acid (10.0%)	OK
Phenol (1.0%)	?
Phosphate Buffer (1.0 M)	OK
Polyethylene Glycol (10%)	OK
Pyridine (100%)	NO
Sodium Carbonate (20%)	OK
Sodium Deoxycholate (5.0%)	OK
Sodium Dodecylsulfate (0.1 M)	OK
Sodium Hydroxide (2.5 M)	NO
Sodium Hypochlorite (200 ppm)	OK
Sodium Nitrate (1.0%)	OK
Sulfamic Acid (5.0%)	OK
Tetrahydrofuran (5.0%)	NO
Toluene (1.0%)	NO
Trifluoroacetic Acid (10%)	OK
Tween 20 (0.1%)	OK
Triton X-100 (0.1%)	OK
Urea (8 M)	OK

OK = Acceptable ? = Questionable NO = Not recommended

COPYRIGHT AND REGISTERED TRADEMARKS

Copyright by Sartorius Stedim Biotech GmbH, Goettingen, Germany. This information has been reprinted with the permission of Sartorius Stedim Biotech GmbH. Vivaspin® is a registered trademark of Sartorius Stedim Biotech GmbH, Goettingen, Germany. Tween® is a registered trademark of Croda International PLC. Triton® is a registered trademark of the Dow Chemical Company.

STORAGE AND STABILITY

Vivaspin® ultrafiltration spin columns should be stored at room temperature. The devices should be used before the expiration date.

ORDERING INFORMATION

Cat. Code	Description
AA022	Vivaspin® 2mL Ultrafiltration Device

Order online anytime at www.bangslabs.com.